


## Measurement Conditions

**Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E**

Integration time: 30 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13908 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

## Spectrum PFCL A

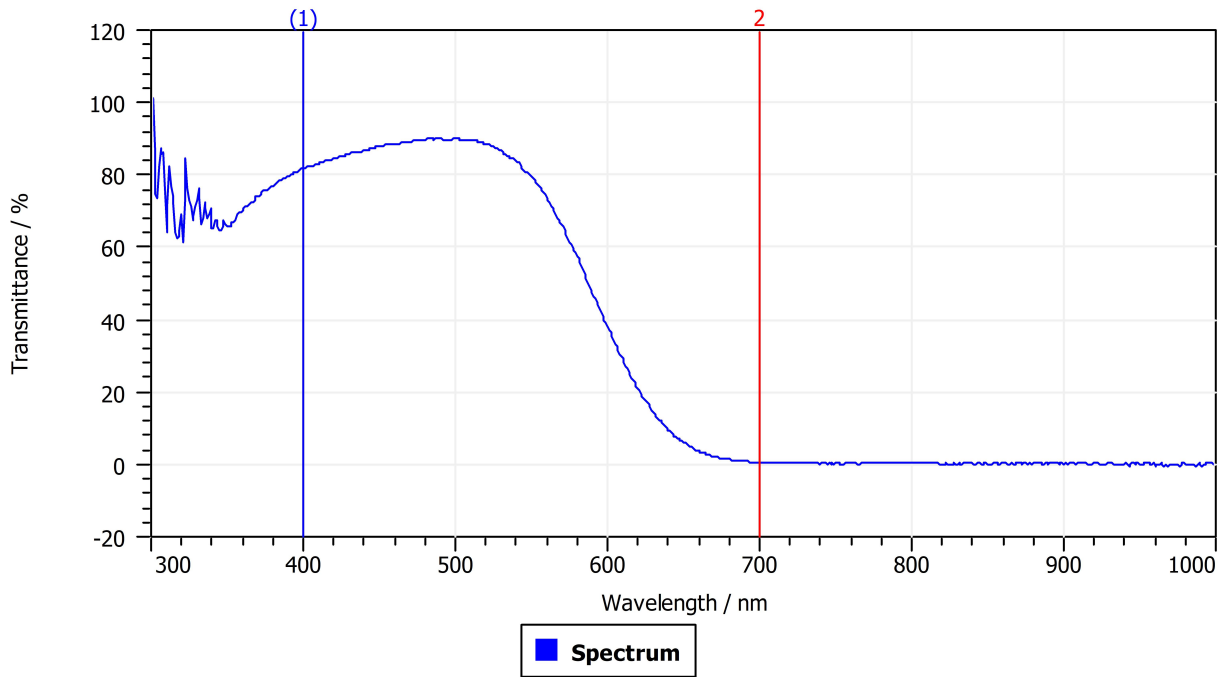

## Results

Y Tau%	68,71	<b>Color coordinates:</b>	x:	0,2411
Peak WL:	301,00 nm		y:	0,3206
Peak Transmission:	1,01		u:	0,1515
Width 50%:	0,00 nm		v:	0,3022
Width 10%:	0,00 nm		u':	0,1515
Width 1%:	0,00 nm		v':	0,4533

### L\*a\*b\*

L\*: 86,361  
a\*: -32,783  
b\*: -14,827  
Ca\*b\*: -35,98  
Ha\*b\*: -204,34

### L\*u\*v\*

L\*: 86,361  
u\*: -52,011  
v\*: -18,204  
Cu\*v\*: -86,361  
Hu\*v\*: -32,783

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\BG38.ISD

Date: 25/10/2019 11:08:08