


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 54 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13731 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

## Spectrum PFCL B

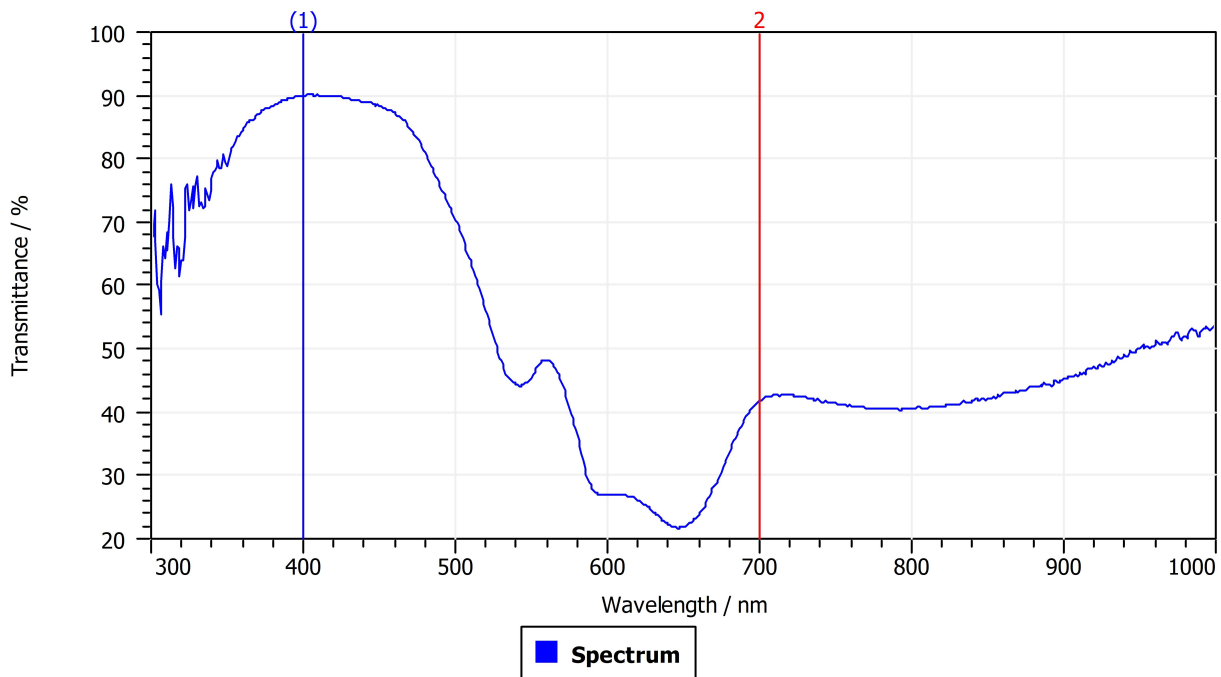

## Results

Y Tau%	47,55	<b>Color coordinates:</b>	x:	0,2302
Peak WL:	403,90 nm		y:	0,2613
Peak Transmission:	0,90		u:	0,1623
Width 50%:	0,00 nm		v:	0,2762
Width 10%:	0,00 nm		u':	0,1623
Width 1%:	0,00 nm		v':	0,4144

### L\*a\*b\*

L\*: 74,542  
a\*: -9,4241  
b\*: -34,257  
Ca\*b\*: -35,53  
Ha\*b\*: -254,62

### L\*u\*v\*

L\*: 74,542  
u\*: -34,491  
v\*: -53,458  
Cu\*v\*: -74,542  
Hu\*v\*: -9,4241

### Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\Filtro\_B.ISD

Date: 25/10/2019 10:32:27