


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	231 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	44 % 13662 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0,1 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

## Spectrum PFCL IR2 800

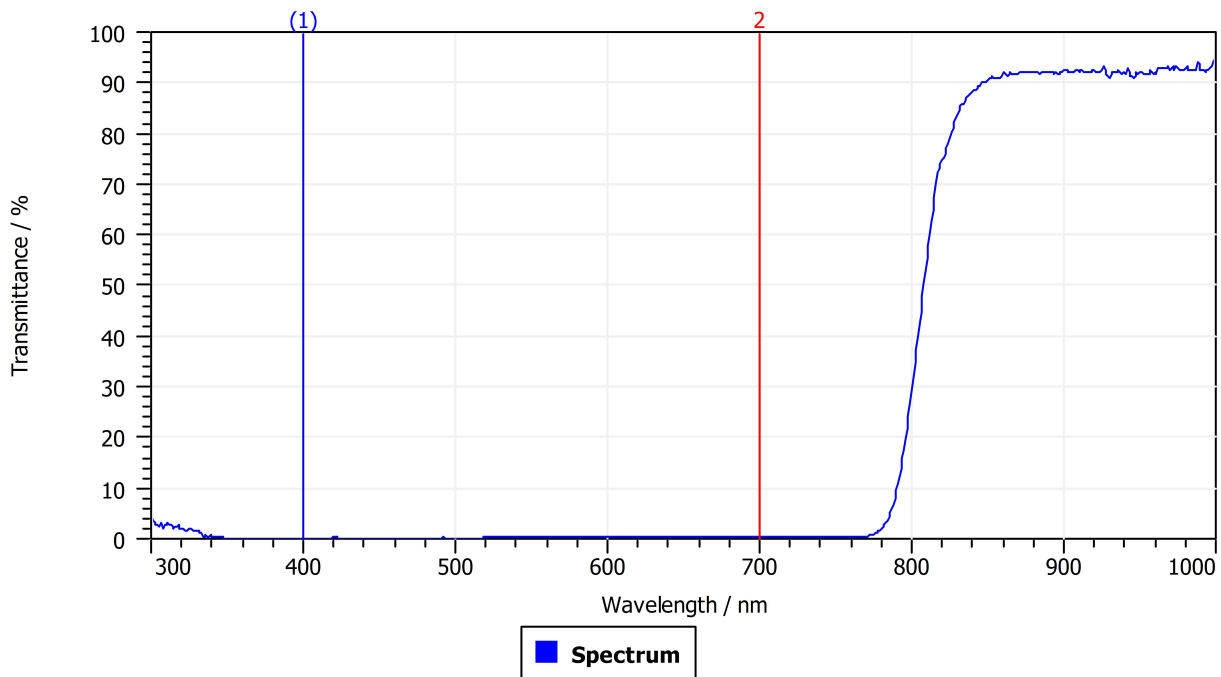

## Results

Y Tau%	0,2139	<b>Color coordinates:</b>	x:	0,3383
Peak WL:	999,00 nm		y:	0,3461
Peak Transmission:	0,94		u:	0,2090
Width 50%:	0,00 nm		v:	0,3206
Width 10%:	0,00 nm		u':	0,2090
Width 1%:	0,00 nm		v':	0,4810

### L\*a\*b\*

L\*: 1,9325  
a\*: 0,2586  
b\*: 0,50156  
Ca\*b\*: -0,5643  
Ha\*b\*: -62,725

### L\*u\*v\*

L\*: 1,9325  
u\*: 0,279  
v\*: 0,28698  
Cu\*v\*: -1,9325  
Hu\*v\*: 0,2586

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\HB800.ISD

Date: 25/10/2019 11:04:31