


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	1000 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	5 % 1676 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0,3 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

Spectrum PFCL IR3 950

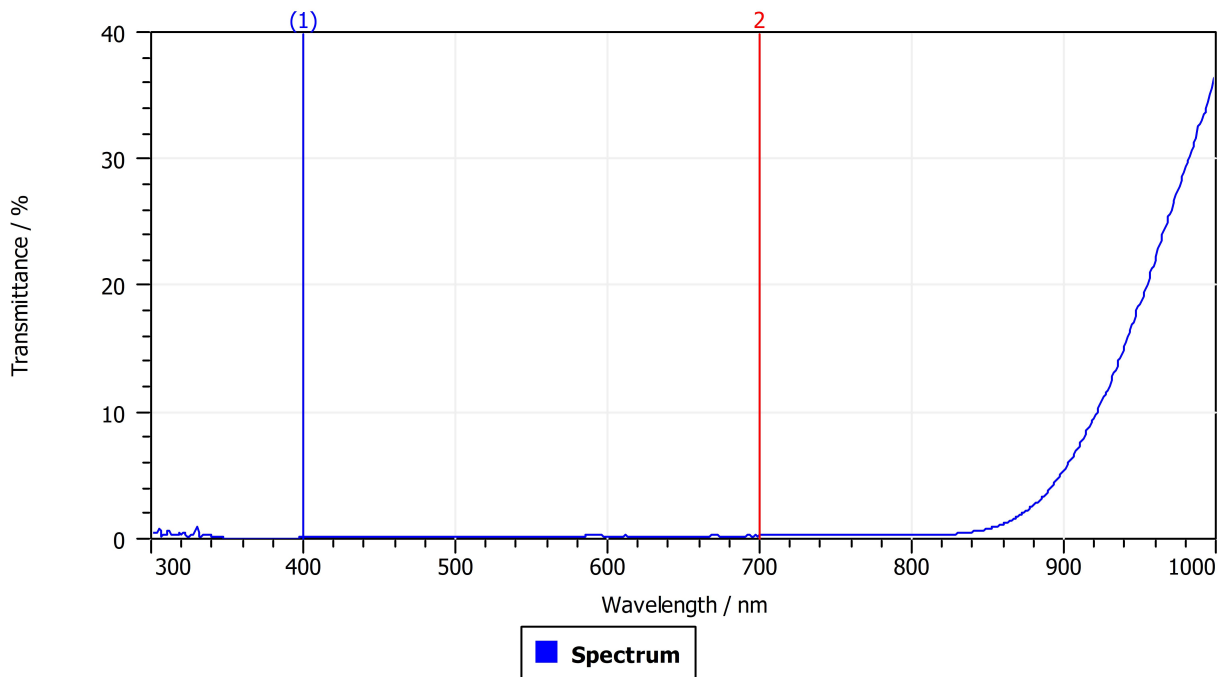

Results

Y Tau%	0,2173	Color coordinates:	x:	0,3347
Peak WL:	999,00 nm		y:	0,3458
Peak Transmission:	0,36		u:	0,2066
Width 50%:	0,00 nm		v:	0,3202
Width 10%:	0,00 nm		u':	0,2066
Width 1%:	0,00 nm		v':	0,4803

L*a*b*

L*: -1,963
a*: 0,17538
b*: 0,47149
Ca*b*: -0,50306
Ha*b*: -69,597

L*u*v*

L*: 1,963
u*: 0,22261
v*: 0,27424
Cu*v*: -1,963
Hu*v*: 0,17538

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure_Filtri\HWB4.ISD

Date: 25/10/2019 11:06:20