


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 678 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13981 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,2 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum PFCL UV Fluo

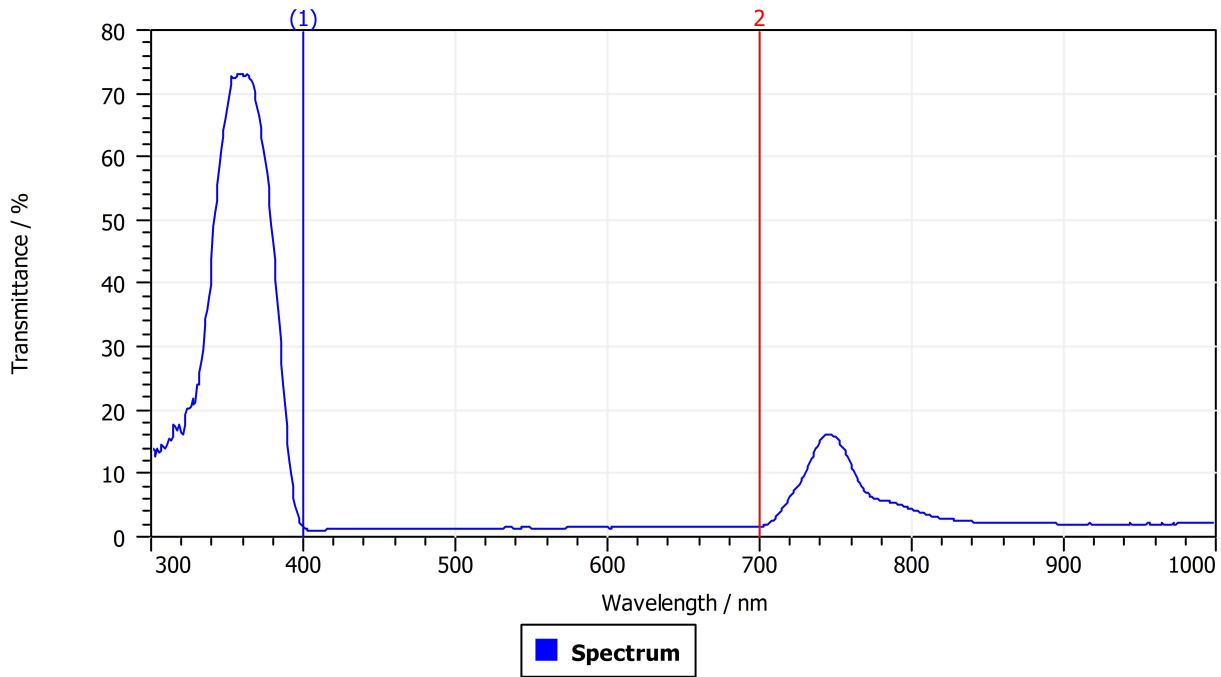

Results

Y Tau%	1,386	Color coordinates:	x:	0,3311
Peak WL:	360,03 nm		y:	0,3467
Peak Transmission:	0,73		u:	0,2038
Width 50%:	45,88 nm		v:	0,3201
Width 10%:	0,00 nm		u':	0,2038
Width 1%:	0,00 nm		v':	0,4802

L*a*b*

L*: 11,865
a*: 0,28666
b*: 2,2498
Ca*b*: -2,2679
Ha*b*: -82,739

L*u*v*

L*: 11,865
u*: 0,91546
v*: 1,6409
Cu*v*: -11,865
Hu*v*: 0,28666

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure_Filtri\ZWB2.ISD

Date: 25/10/2019 10:49:27