


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 674 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13740 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,2 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum PFCL UV Fluo

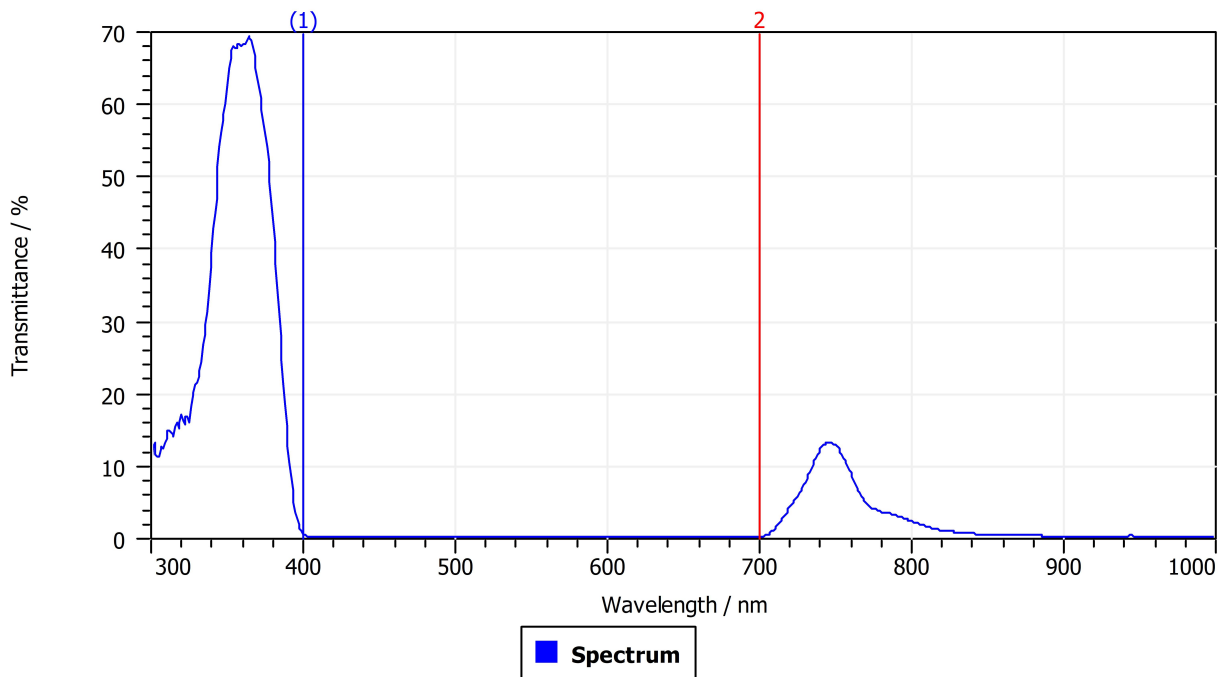

Results

Y Tau%	0,1857	Color coordinates:	x:	0,3227
Peak WL:	363,37 nm		y:	0,3260
Peak Transmission:	0,69		u:	0,2060
Width 50%:	44,80 nm		v:	0,3121
Width 10%:	0,00 nm		u':	0,2060
Width 1%:	0,00 nm		v':	0,4682

L*a*b*

L*:	1,6774
a*:	0,31985
b*:	-0,011574
Ca*b*:	-0,32006
Ha*b*:	-357,93

L*u*v*

L*:	1,6774
u*:	0,17802
v*:	-0,029204
Cu*v*:	-1,6774
Hu*v*:	0,31985

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure_Filtri\ZBW2_100X100.ISD

Date: 25/10/2019 10:57:27