


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 464 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 44 % 13662 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,2 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

## Spectrum PFCL UV HMI

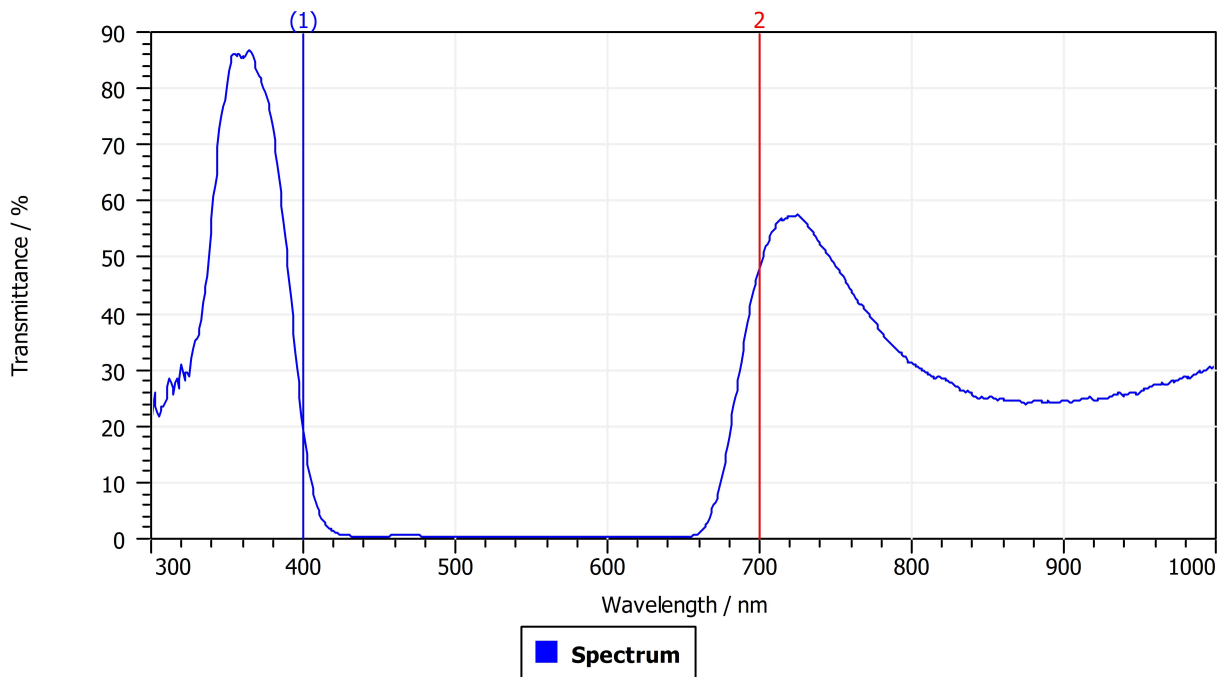

## Results

Y Tau%	0,3218	<b>Color coordinates:</b>	x:	0,3017
Peak WL:	364,02 nm		y:	0,1899
Peak Transmission:	0,87		u:	0,2581
Width 50%:	56,82 nm		v:	0,2437
Width 10%:	0,00 nm		u':	0,2581
Width 1%:	0,00 nm		v':	0,3656

### L\*a\*b\*

L\*: -2,907  
a\*: 8,4656  
b\*: -7,486  
Ca\*b\*: -11,301  
Ha\*b\*: -318,51

### L\*u\*v\*

L\*: 2,907  
u\*: 2,2782  
v\*: -3,928  
Cu\*v\*: -2,907  
Hu\*v\*: 8,4656

### Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\ZBW3\_100X100.ISD

Date: 25/10/2019 10:59:50