


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 472 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 44 % 13680 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,2 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum PFCL UV HMI

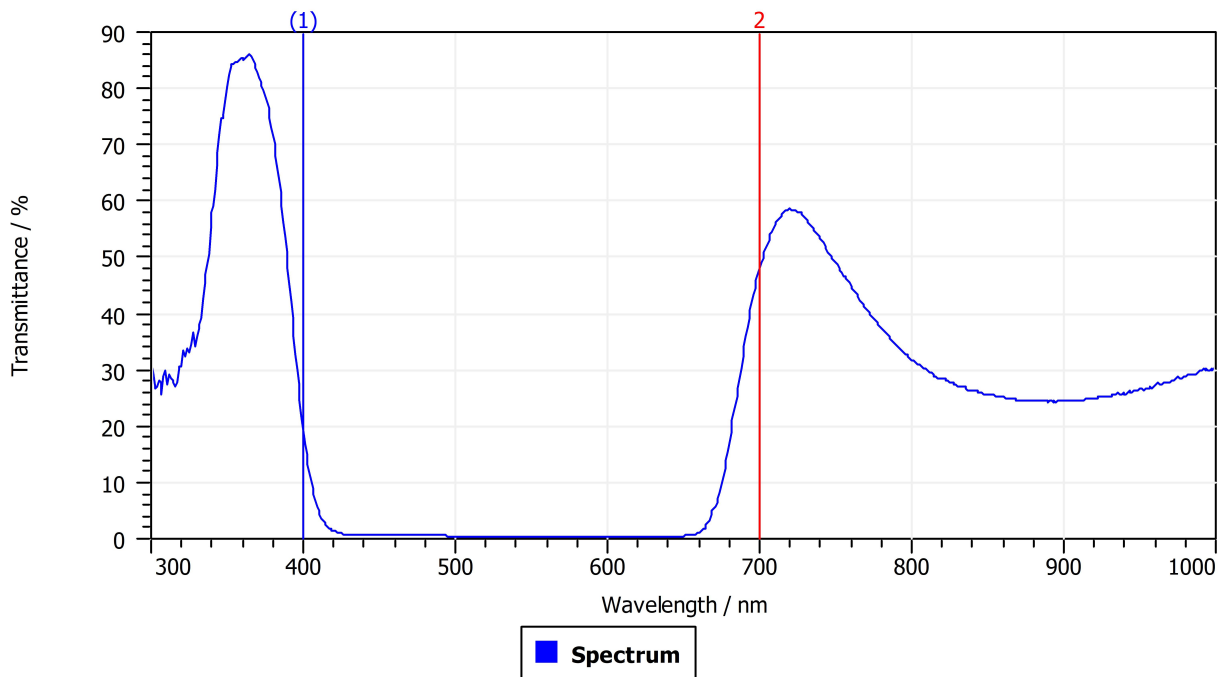

Results

Y Tau%	0,5156	Color coordinates:	x:	0,3131
Peak WL:	363,60 nm		y:	0,2327
Peak Transmission:	0,86		u:	0,2424
Width 50%:	57,55 nm		v:	0,2703
Width 10%:	0,00 nm		u':	0,2424
Width 1%:	0,00 nm		v':	0,4054

L*a*b*

L*: 4,6571
a*: 8,4055
b*: -6,5567
Ca*b*: -10,66
Ha*b*: -322,04

L*u*v*

L*: 4,6571
u*: 2,6946
v*: -3,8828
Cu*v*: -4,6571
Hu*v*: 8,4055

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure_Filtri\ZWB3_spessoremagg.ISD

Date: 25/10/2019 11:20:24