


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 27 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 44 % 13638 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

## Spectrum PFCL XA

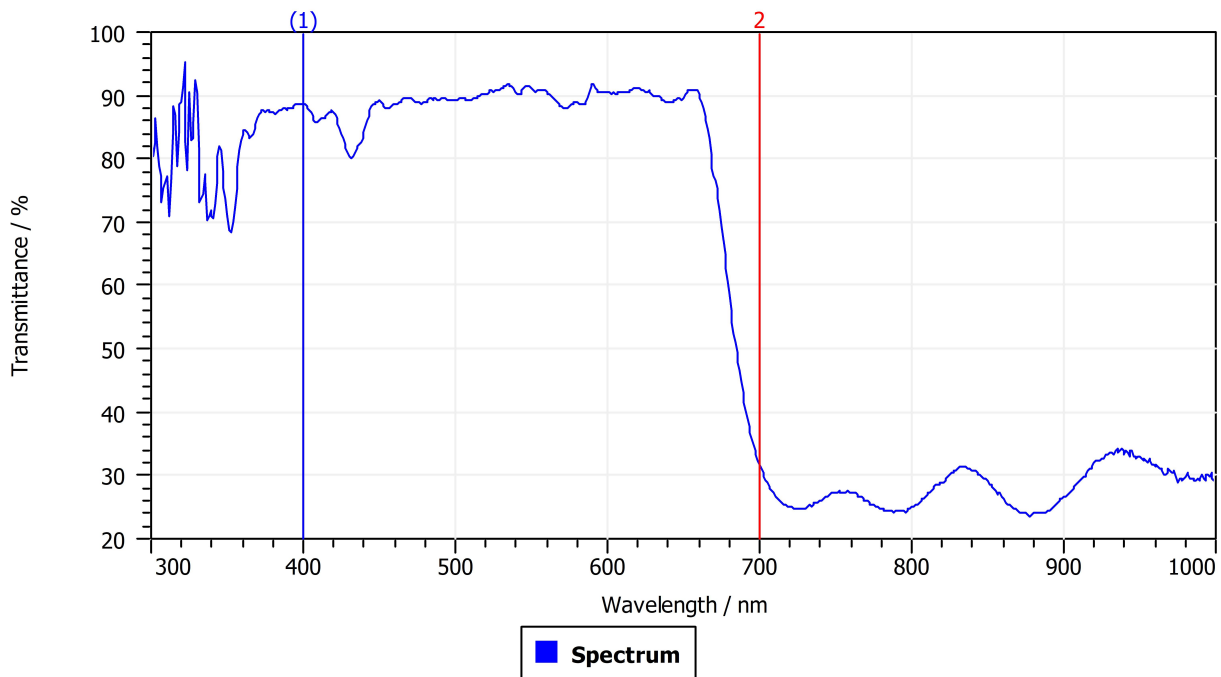

## Results

Y Tau%	89,88	<b>Color coordinates:</b>	x:	0,3156
Peak WL:	321,42 nm		y:	0,3355
Peak Transmission:	0,93		u:	0,1974
Width 50%:	0,00 nm		v:	0,3148
Width 10%:	0,00 nm		u':	0,1974
Width 1%:	0,00 nm		v':	0,4722

### L\*a\*b\*

L\*: 95,948  
a\*: -1,288  
b\*: 2,024  
Ca\*b\*: -2,3991  
Ha\*b\*: -122,47

### L\*u\*v\*

L\*: 95,948  
u\*: -0,5862  
v\*: 3,3125  
Cu\*v\*: -95,948  
Hu\*v\*: -1,288

### Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\FiltroX\_A.ISD

Date: 25/10/2019 10:46:26