


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	123 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	46 % 14084 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0,1 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

## Spectrum PFCL XB

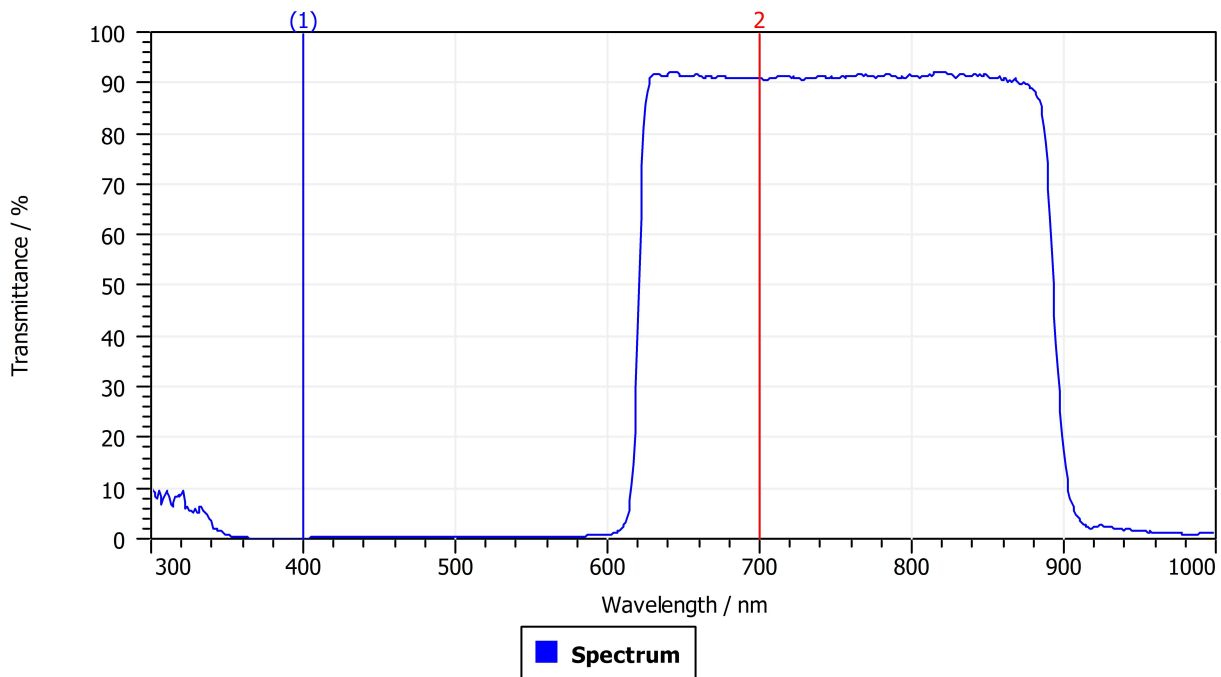

## Results

Y Tau%	6,196	<b>Color coordinates:</b>	x:	0,6830
Peak WL:	819,33 nm		y:	0,3031
Peak Transmission:	0,92		u:	0,5183
Width 50%:	273,22 nm		v:	0,3450
Width 10%:	287,64 nm		u':	0,5183
Width 1%:	379,16 nm		v':	0,5175

### L\*a\*b\*

L\*: 29,901  
a\*: 66,184  
b\*: 47,439  
Ca\*b\*: -81,429  
Ha\*b\*: -35,632

### L\*u\*v\*

L\*: 29,901  
u\*: 124,56  
v\*: 18,652  
Cu\*v\*: -29,901  
Hu\*v\*: 66,184

### Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\FiltroX\_B.ISD

Date: 25/10/2019 10:45:16