


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 111 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13798 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum PFCL XC

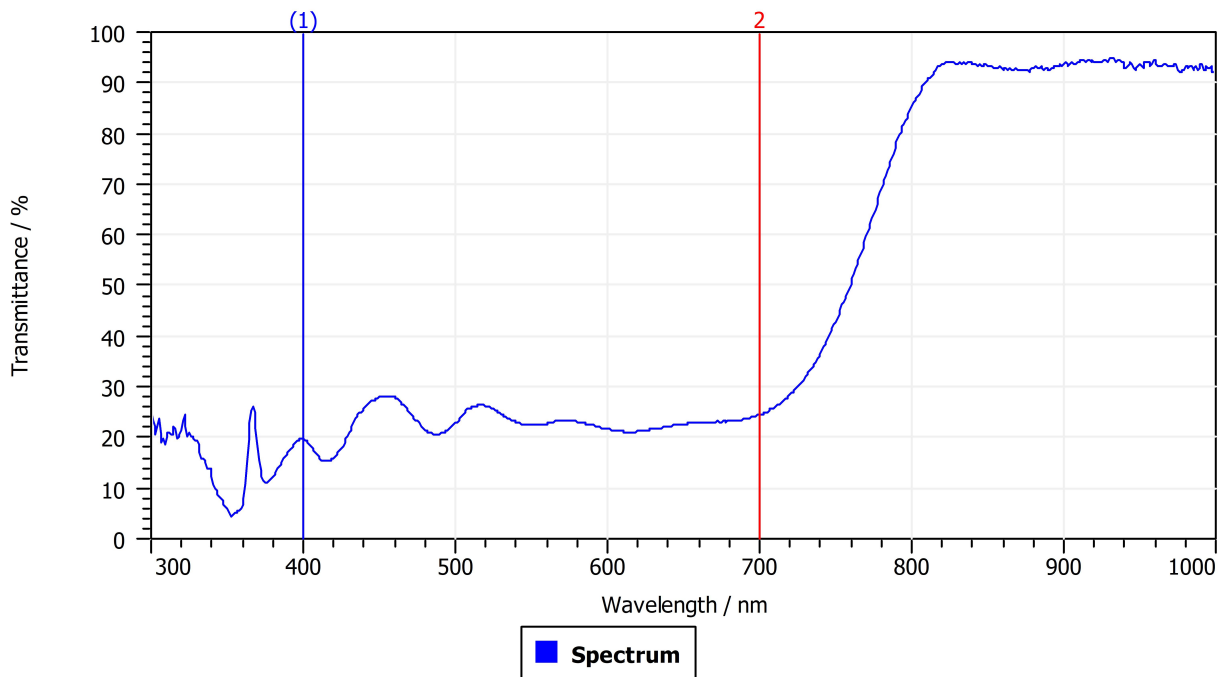

Results

Y Tau%	23,22	Color coordinates:	x:	0,3046
Peak WL:	930,79 nm		y:	0,3275
Peak Transmission:	0,95		u:	0,1927
Width 50%:	0,00 nm		v:	0,3109
Width 10%:	0,00 nm		u':	0,1927
Width 1%:	0,00 nm		v':	0,4663

L*a*b*

L*: 55,295
a*: -1,9883
b*: -1,8766
Ca*b*: -2,734
Ha*b*: -223,34

L*u*v*

L*: 55,295
u*: -3,6928
v*: -2,2987
Cu*v*: -55,295
Hu*v*: -1,9883

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure_Filtri\FiltroX_C.ISD

Date: 25/10/2019 10:42:24