


## Measurement Conditions

**Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E**

Integration time: 27 ms	Averages: 20
Density filter: none	Serial number: 236514212
Signal level: 45 % 13837 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0,0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

## Spectrum PFCL X UV IR cut

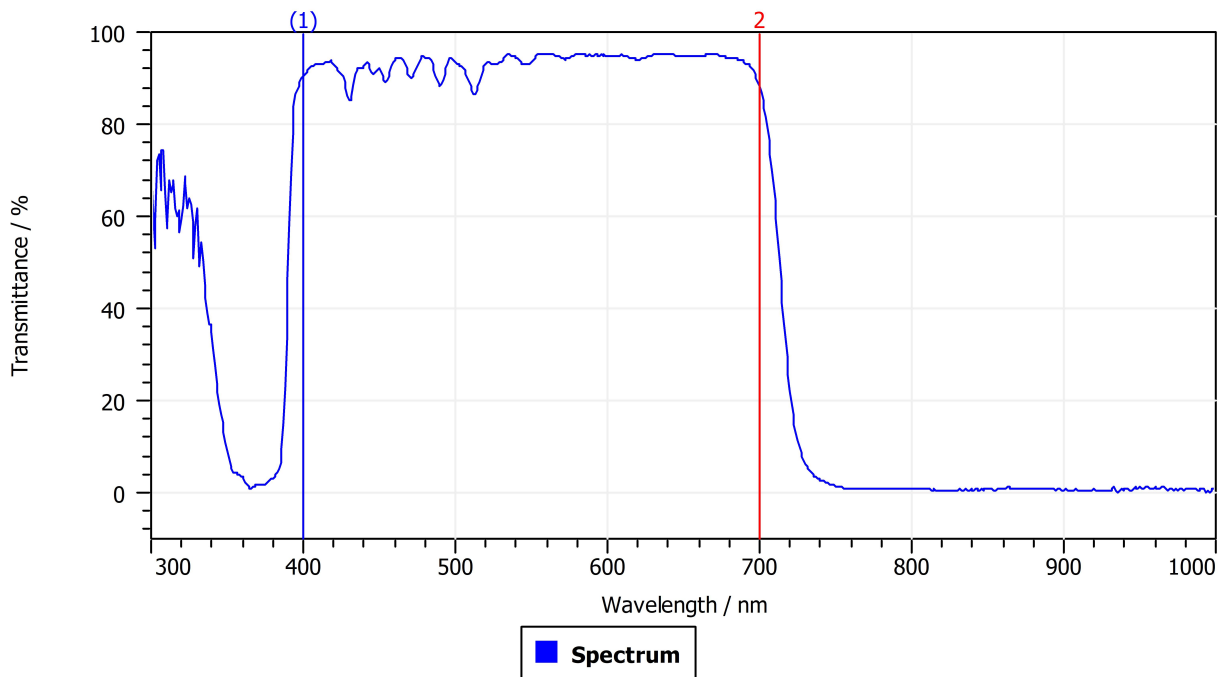

## Results

Y Tau%	93,7	<b>Color coordinates:</b>	x:	0,3170
Peak WL:	581,93 nm		y:	0,3331
Peak Transmission:	0,95		u:	0,1993
Width 50%:	323,55 nm		v:	0,3141
Width 10%:	340,31 nm		u':	0,1993
Width 1%:	0,00 nm		v':	0,4711

### L\*a\*b\*

L\*: 97,511  
a\*: 0,59888  
b\*: 1,3905  
Ca\*b\*: -1,514  
Ha\*b\*: -66,699

### L\*u\*v\*

L\*: 97,511  
u\*: 1,7741  
v\*: 2,0145  
Cu\*v\*: -97,511  
Hu\*v\*: 0,59888

Comment:

File name: C:\Users\Laptop-01\Desktop\Misure\_Filtri\FiltroX\_UVIRCut.ISD

Date: 25/10/2019 10:40:39