


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	10 ms	Averages:	20
Density filter:	OD1	Serial number:	236514212
Signal level:	23 % 6939 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

Spectrum

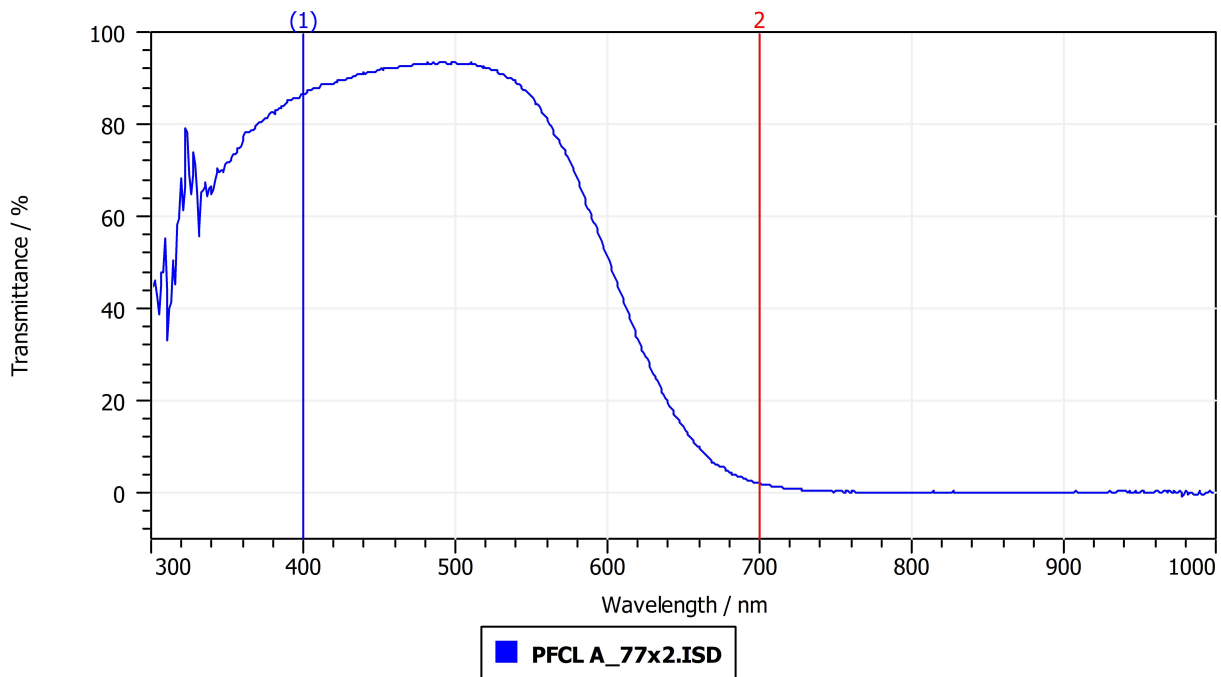

Results

Y Tau%	76,01	Color coordinates:	x:	0,2568
Peak WL:	491,87 nm		y:	0,3242
Peak Transmission:	0,93		u:	0,1611
Width 50%:	288,76 nm		v:	0,3051
Width 10%:	0,00 nm		u':	0,1611
Width 1%:	0,00 nm		v':	0,4576

L*a*b*

L*: 89,863
a*: -26,577
b*: -11,652
Ca*b*: -29,019
Ha*b*: -203,67

L*u*v*

L*: 89,863
u*: -42,995
v*: -13,962
Cu*v*: -89,863
Hu*v*: -26,577

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL A_77x2.ISD

Date: 26/03/2021 14:50:58