


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	35 ms	Averages:	20
Density filter:	OD1	Serial number:	236514212
Signal level:	45 % 13920 Counts	CCD temperature:	-10,18 °C
Analysis range	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

Spectrum

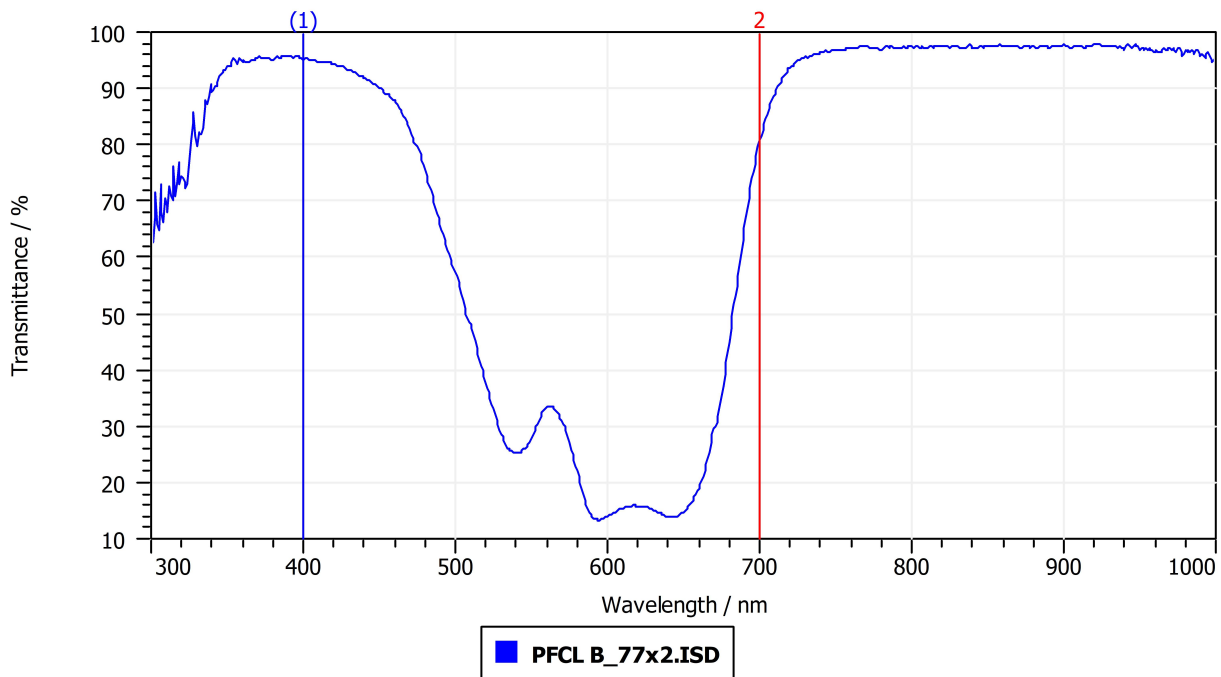

Results

Y Tau%	33,61	Color coordinates:	x:	0,2034
Peak WL:	836,84 nm		y:	0,2119
Peak Transmission:	0,97		u:	0,1584
Width 50%:	0,00 nm		v:	0,2475
Width 10%:	0,00 nm		u':	0,1584
Width 1%:	0,00 nm		v':	0,3713

L*a*b*

L*: 64,651
a*: 1,4524
b*: -51,451
Ca*b*: -51,472
Ha*b*: -271,62

L*u*v*

L*: 64,651
u*: -33,137
v*: -82,566
Cu*v*: -64,651
Hu*v*: 1,4524

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL B_77x2.ISD

Date: 29/03/2021 09:40:28