


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	10 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	79 % 24317 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

## Spectrum

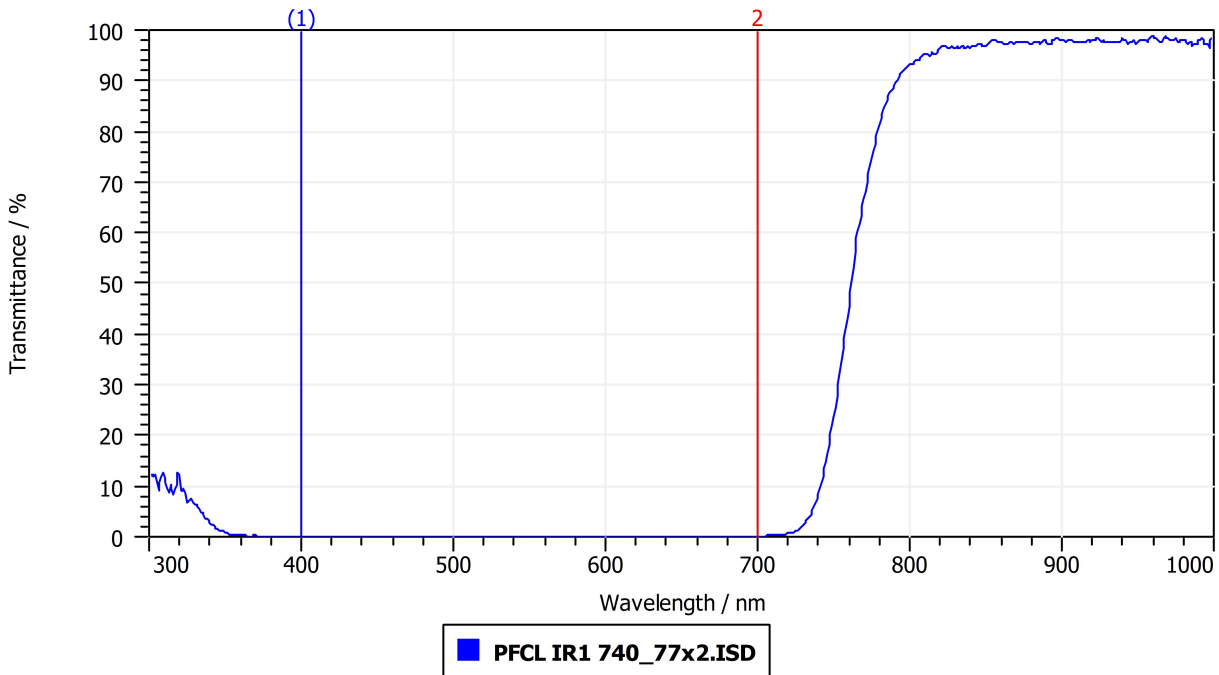

## Results

Y Tau%	0,02042	<b>Color coordinates:</b>	x:	0,3473
Peak WL:	969,29 nm		y:	0,3064
Peak Transmission:	0,99		u:	0,2323
Width 50%:	0,00 nm		v:	0,3073
Width 10%:	0,00 nm		u':	0,2323
Width 1%:	0,00 nm		v':	0,4610

### L\*a\*b\*

L\*: ,18447  
a\*: 0,15558  
b\*: -0,016838  
Ca\*b\*: -0,15648  
Ha\*b\*: -353,82

### L\*u\*v\*

L\*: 0,18447  
u\*: 0,082495  
v\*: -0,02053  
Cu\*v\*: -0,18447  
Hu\*v\*: 0,15558

### Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL IR1 740\_77x2.ISD

Date: 26/03/2021 15:03:18