


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	10 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	52 % 16102 Counts	CCD temperature:	-10,18 °C
Analysis range	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

## Spectrum

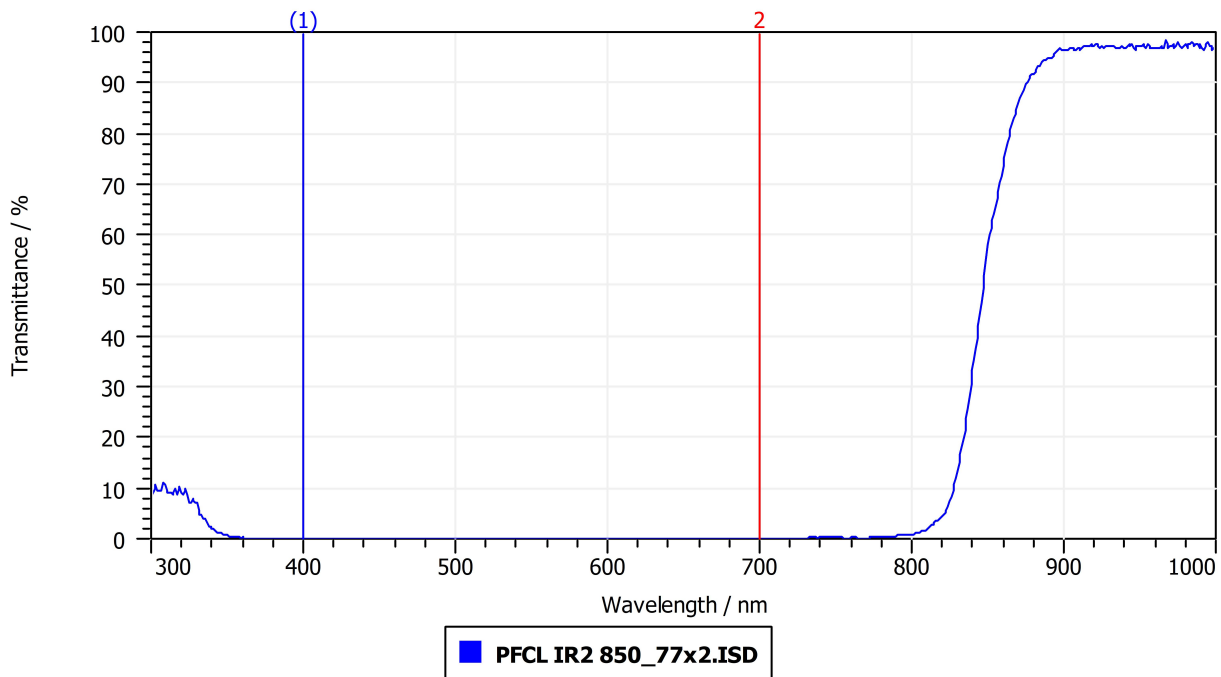

## Results

Y Tau%	0,01304	<b>Color coordinates:</b>	x:	0,3225
Peak WL:	969,19 nm		y:	0,3043
Peak Transmission:	0,97		u:	0,2148
Width 50%:	0,00 nm		v:	0,3040
Width 10%:	0,00 nm		u':	0,2148
Width 1%:	0,00 nm		v':	0,4559

### L\*a\*b\*

L*:	,11777	L*:	0,11777
a*:	0,059924	u*:	0,025946
b*:	-0,02901	v*:	-0,020828
Ca*b*:	-0,066577	Cu*v*:	-0,11777
Ha*b*:	-334,17	Hu*v*:	0,059924

### L\*u\*v\*

### Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL IR2 850\_77x2.ISD

Date: 26/03/2021 14:43:55