


## Measurement Conditions

### Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	76 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	45 % 13803 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

## Spectrum

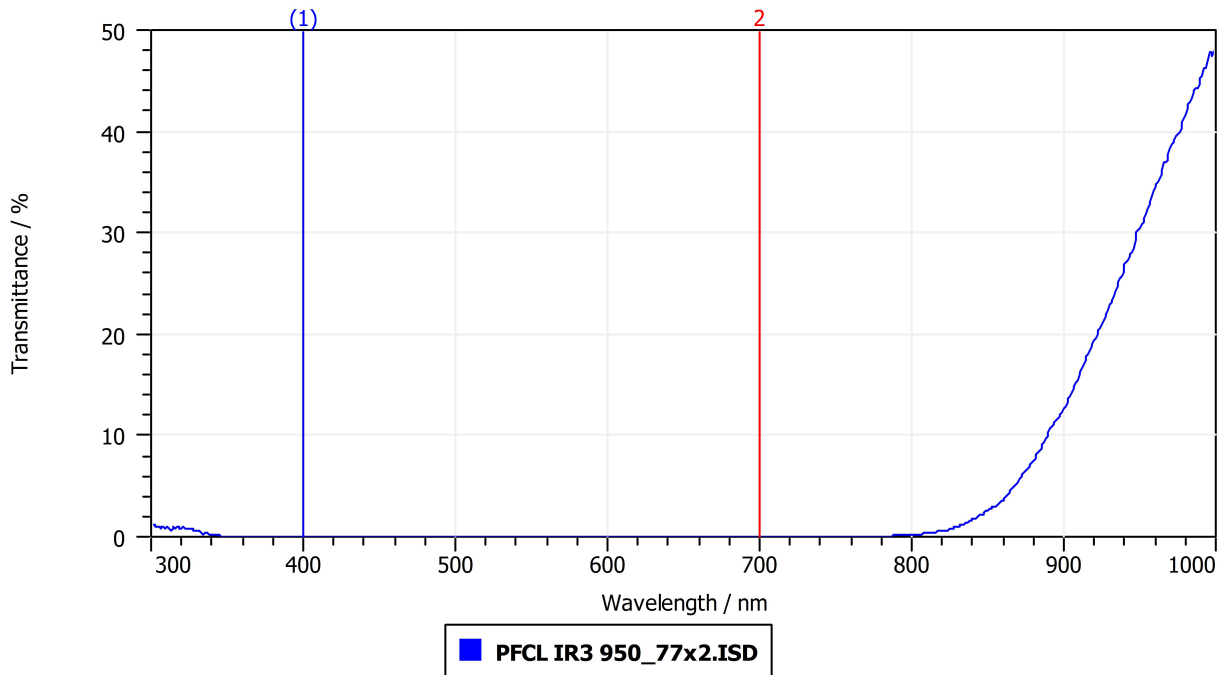

## Results

Y Tau%	0,001484	<b>Color coordinates:</b>	x:	0,3422
Peak WL:	999,00 nm		y:	0,3176
Peak Transmission:	0,48		u:	0,2234
Width 50%:	0,00 nm		v:	0,3110
Width 10%:	0,00 nm		u':	0,2234
Width 1%:	0,00 nm		v':	0,4666

### L\*a\*b\*

L*:	013407	L*:	0,013407
a*:	0,0078887	u*:	0,0044586
b*:	4,9692E-00	v*:	-0,0005197
Ca*b*:	-0,0078889	Cu*v*:	-0,013407
Ha*b*:	-0,36091	Hu*v*:	0,0078887

### L\*u\*v\*

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL IR3 950\_77x2.ISD

Date: 26/03/2021 14:47:05