


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 10 ms	Averages: 20
Density filter: OD1	Serial number: 236514212
Signal level: 23 % 7065 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum

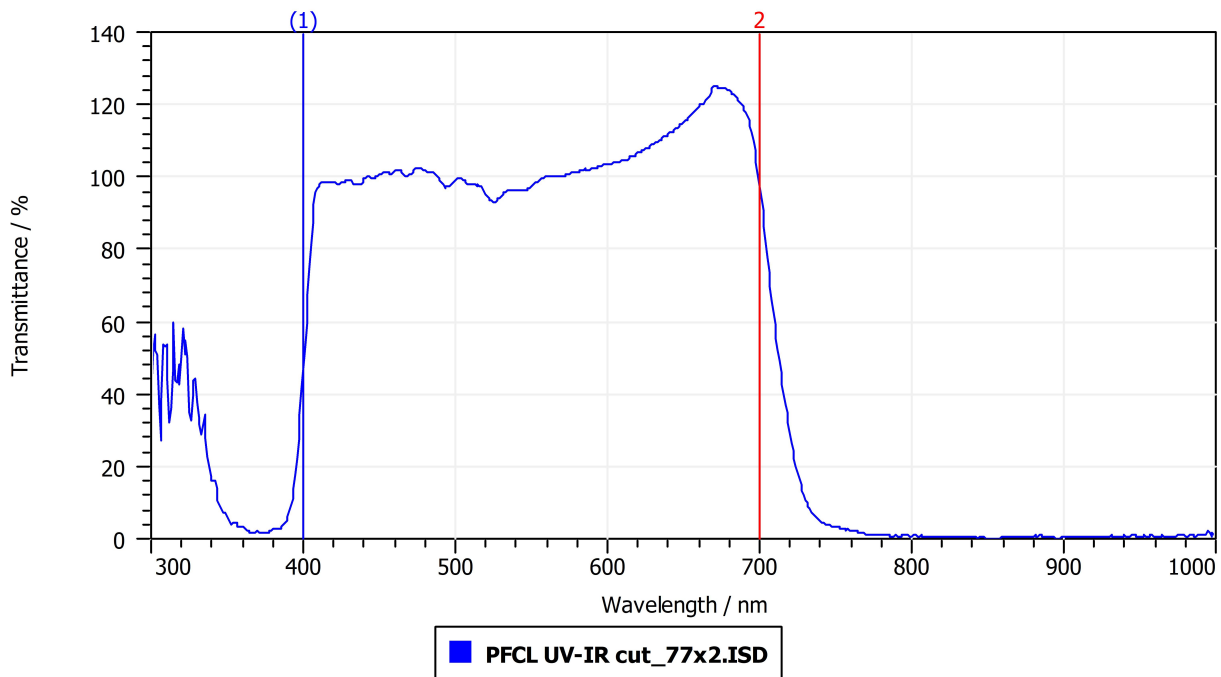

Results

Y Tau%	99,97	Color coordinates:	x:	0,3195
Peak WL:	672,65 nm		y:	0,3288
Peak Transmission:	1,25		u:	0,2027
Width 50%:	306,63 nm		v:	0,3128
Width 10%:	335,09 nm		u':	0,2027
Width 1%:	0,00 nm		v':	0,4692

L*a*b*

L*: 99,987
a*: 4,1287
b*: 0,24031
Ca*b*: -4,1357
Ha*b*: -3,3311

L*u*v*

L*: 99,987
u*: 6,2582
v*: -0,38474
Cu*v*: -99,987
Hu*v*: 4,1287

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL UV-IR cut_77x2.ISD

Date: 26/03/2021 12:56:07