


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time: 10 ms	Averages: 20
Density filter: OD1	Serial number: 236514212
Signal level: 23 % 7155 Counts	CCD temperature: -10,18 °C
Analysis range 300 - 1000 nm	Last dark current: 0 min
Illuminant ref.: Illuminant D65 (0,3138;0,3310)	
Skiplevel:	Observer: 10 °

Spectrum

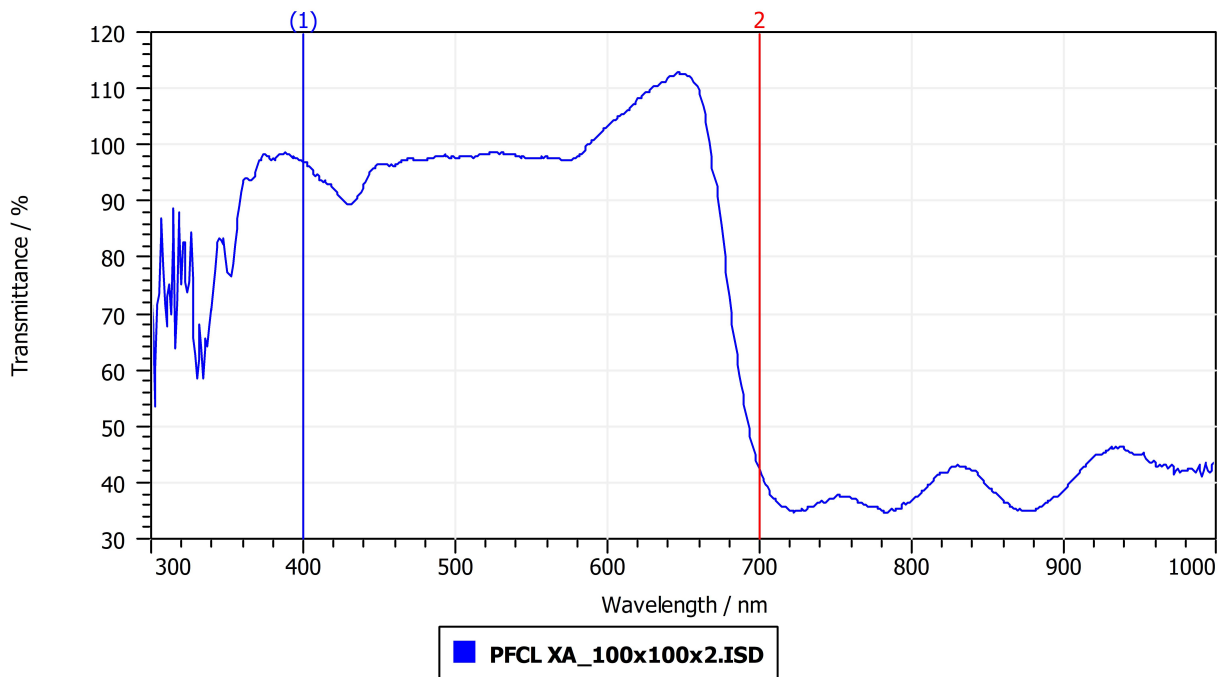

Results

Y Tau%	99,34	Color coordinates:	x:	0,3213
Peak WL:	647,71 nm		y:	0,3350
Peak Transmission:	1,13		u:	0,2016
Width 50%:	386,10 nm		v:	0,3152
Width 10%:	0,00 nm		u':	0,2016
Width 1%:	0,00 nm		v':	0,4727

L*a*b*

L*: 99,742
a*: 1,9611
b*: 2,9613
Ca*b*: -3,5518
Ha*b*: -56,485

L*u*v*

L*: 99,742
u*: 4,81
v*: 4,1572
Cu*v*: -99,742
Hu*v*: 1,9611

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL XA_100x100x2.ISD

Date: 26/03/2021 11:53:20