


Measurement Conditions

Measurement setup: CAS 140B/CT(S)/D, CAS 120, MAS 40 - 2365142E

Integration time:	89 ms	Averages:	20
Density filter:	none	Serial number:	236514212
Signal level:	45 % 13854 Counts	CCD temperature:	-10,18 °C
Analysis range:	300 - 1000 nm	Last dark current:	0 min
Illuminant ref.:	Illuminant D65 (0,3138;0,3310)		
Skiplevel:		Observer:	10 °

Spectrum

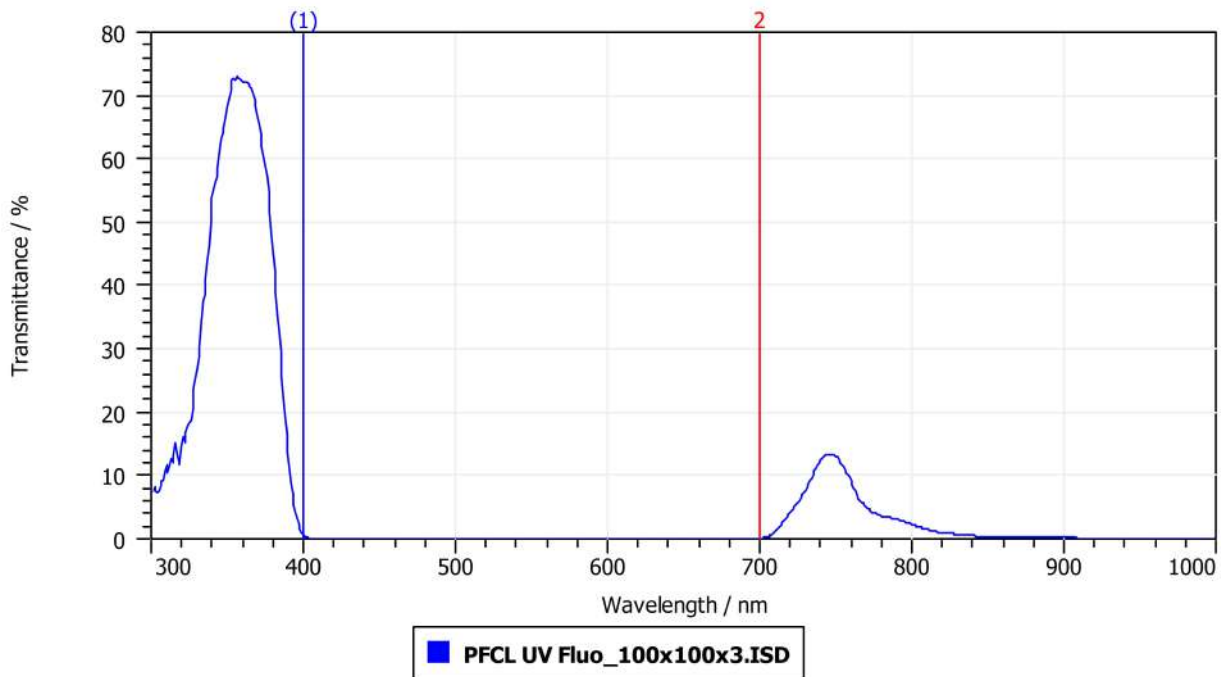

Results

Y Tau%	0,005042	Color coordinates:	x:	0,2210
Peak WL:	356,58 nm		y:	0,1162
Peak Transmission:	0,73		u:	0,2236
Width 50%:	49,03 nm		v:	0,1764
Width 10%:	0,00 nm		u':	0,2236
Width 1%:	0,00 nm		v':	0,2646

L*a*b*

L*: 045542
a*: 0,19738
b*: -0,33876
Ca*b*: -0,39207
Ha*b*: -300,23

L*u*v*

L*: 0,045542
u*: 0,015253
v*: -0,12133
Cu*v*: -0,045542
Hu*v*: 0,19738

Comment:

File name: C:\Users\Laptop-01\Desktop\MISURE CAS\Optical filters\Filters\PFCL UV Fluo_100x100x3.ISD
Date: 26/03/2021 12:10:07